

NAD/NADH Microplate Assay Kit

Cat #: orb219864 (manual)

Detection and Quantification of NAD/NADH Content in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.

INTRODUCTION

Nicotinamide adenine dinucleotide (NAD⁺) is a vital coenzyme found in all cells. As NAD⁺ is involved in redox reactions, it is found in two forms in cells. NAD⁺ is an oxidizing agent and becomes reduced to form NADH, which can be used as a reducing agent. As a result, it plays a key role in metabolism and other cellular processes. In organisms, NAD⁺ can be synthesized de novo from tryptophan or aspartic acid. Because of the wide variety of functions that NAD⁺ plays, it is a popular target for pharmaceuticals. NAD/NADH Microplate Assay Kit provides a simple and direct procedure for measuring NAD⁺/NADH levels in a variety of samples. The kit is based on an alcohol dehydrogenase cycling reaction, in which the formed NADH reduces a formazan reagent. The intensity of the reduced product color, measured at 450 nm, is proportionate to the NAD⁺/NADH concentration in the sample.

KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 2	4 °C
Reaction Buffer	10 ml x 1	4 °C
Enzyme	Powder x 1	-20 °C
Substrate	10 ml x 1	4 °C
Dye Reagent A	Powder x 1	4 °C
Dye Reagent B	1 ml x 1	4 °C
Standard	Powder x 1	-20 °C, keep in dark
Technical Manual	1 Manual	

Note:

Dye Reagent A: add 1 ml distilled water to dissolve before use, mix. Store at -20°C for a month.

Enzyme: add 1 ml Reaction Buffer to dissolve before use, mix. Store at -80°C for a month.

Standard: add 1 ml distilled water to dissolve, mix; then add 25 µl solution into 975 µl distilled water, mix.

The concentration will be 50 µmol/L. Store at -20°C for a month.

MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 450 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Ice
7. Centrifuge
8. Timer
9. Water bath

SAMPLE PREPARATION

1. For serum or plasma samples

Total NADH and NAD⁺:

Detect directly or dilute with distilled water.

NAD⁺ Decomposition:

To detect NADH, the NAD⁺ needs to be decomposed before the reaction. Keep some samples at 60 °C for 30 min in water bath to completely decompose the NAD⁺. Cool samples on ice. Centrifuge at 8000g 4 °C for 10 minutes and transfer the supernatant into a new centrifuge tube, keep it on ice for detection.

2. For tissue samples

Total NADH and NAD⁺:

Weigh out 0.05 g tissue, homogenize with 500 µl Assay Buffer on ice; centrifuged at 8000g 4 °C for 10 minutes, transfer the supernatant into a new centrifuge tube, keep it on ice for detection.

NAD⁺ Decomposition:

To detect NADH, the NAD⁺ needs to be decomposed before the reaction. Keep some samples at 60 °C for 30 min in water bath to completely decompose the NAD⁺. Cool samples on ice. Centrifuge at 8000g 4 °C for 10 minutes and transfer the supernatant into a new centrifuge tube, keep it on ice for detection.

3. For cell and bacteria samples

Total NADH and NAD⁺:

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 500 µl Assay Buffer for 500×10^4 cell or bacteria, sonicate (with power 20%, sonication 2s, interval 1s, repeat 30

times) ; incubate at 60 °C for 20 minutes; Centrifuge at 8000g 4 °C for 10 minutes and transfer the supernatant into a new centrifuge tube; keep it on ice for detection.

NAD⁺ Decomposition:

To detect NADH, the NAD⁺ needs to be decomposed before the reaction. Keep some samples at 60 °C for 30 min in water bath to completely decompose the NAD⁺. Cool samples on ice. Centrifuge at 8000g 4 °C for 10 minutes and transfer the supernatant into a new centrifuge tube, keep it on ice for detection.

ASSAY PROCEDURE

Add following reagents into the microplate:

Reagent	Sample (Total)	Sample (NADH)	Standard	Blank
Sample	20 μ l	20 μ l	--	--
Standard	--	--	20 μ l	--
Distilled water	--	--	--	20 μ l
Reaction Buffer	70 μ l	70 μ l	70 μ l	70 μ l
Enzyme	10 μ l	10 μ l	10 μ l	10 μ l
Substrate	80 μ l	80 μ l	80 μ l	80 μ l
Dye Reagent A	10 μ l	10 μ l	10 μ l	10 μ l
Dye Reagent B	10 μ l	10 μ l	10 μ l	10 μ l

Mix, keep in dark for 10 minutes at room temperature, record absorbance measured at 450 nm.

Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) The concentrations can vary over a wide range depending on the different samples. For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range.

CALCULATION

1. According to the volume of sample

$$\begin{aligned} \text{NAD/NADH } (\mu\text{mol/ml}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample (Total)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} \\ &= 0.05 \times (\text{OD}_{\text{Sample (Total)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$

$$\begin{aligned} \text{NADH } (\mu\text{mol/ml}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample (NADH)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} \\ &= 0.05 \times (\text{OD}_{\text{Sample (NADH)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$

$$\text{NAD}^+ (\mu\text{mol/ml}) = \text{NAD/NADH } (\mu\text{mol/ml}) - \text{NADH } (\mu\text{mol/ml})$$

2. According to the weight of sample

$$\begin{aligned} \text{NAD/NADH } (\mu\text{mol/g}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample (Total)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (W \times \\ &\quad V_{\text{Sample}} / V_{\text{Assay}}) \\ &= 0.025 \times (\text{OD}_{\text{Sample (Total)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

$$\begin{aligned} \text{NADH } (\mu\text{mol/g}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample (NADH)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (W \times V_{\text{Sample}} / \\ &\quad V_{\text{Assay}}) \\ &= 0.025 \times (\text{OD}_{\text{Sample (NADH)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

$$\text{NAD}^+ (\mu\text{mol/g}) = \text{NAD/NADH } (\mu\text{mol/g}) - \text{NADH } (\mu\text{mol/g})$$

3. According to the quantity of cells or bacteria

$$\begin{aligned} \text{NAD/NADH } (\mu\text{mol}/10^4) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample (Total)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (N \times \\ &\quad V_{\text{Sample}} / V_{\text{Assay}}) \\ &= 0.025 \times (\text{OD}_{\text{Sample (Total)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N \end{aligned}$$

$$\begin{aligned} \text{NADH } (\mu\text{mol}/10^4) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample (NADH)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (N \times V_{\text{Sample}} \\ &\quad / V_{\text{Assay}}) \\ &= 0.025 \times (\text{OD}_{\text{Sample (NADH)}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N \end{aligned}$$

$$\text{NAD}^+ (\mu\text{mol}/10^4) = \text{NAD/NADH } (\mu\text{mol}/10^4) - \text{NADH } (\mu\text{mol}/10^4)$$

C_{Protein} : the protein concentration, mg/ml;

C_{Standard} : the protein concentration, 50 $\mu\text{mol/L}$ = 0.05 $\mu\text{mol/ml}$;

W: the weight of sample, g;

V_{Sample} : the volume of sample, 0.02 ml;


V_{Standard} : the volume of sample, 0.02 ml;

V_{Assay} : the volume of Assay Buffer, 0.5 ml;

N: the quantity of cell or bacteria, $N \times 10^4$.

TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

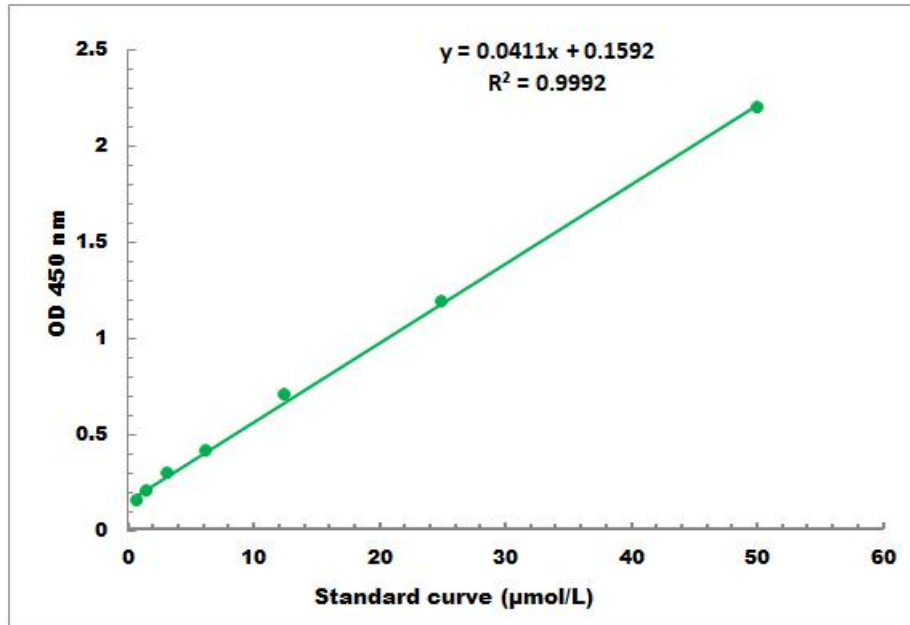

Detection Range: 0.5 µmol/L - 50 µmol/L