

Acetylcholinesterase

Microplate Assay Kit

Cat #: orb390774 (manual)

Detection and Quantification of Acetylcholinesterase (AChE) Activity in Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.

INTRODUCTION

Acetylcholinesterases (AChEs) are enzymes that hydrolyze the neurotransmitter acetylcholine (ACh) to and choline. AChE is located at the synaptic cleft and functions to terminate synaptic transmission by catalyzing the breakdown of ACh allowing cholinergic neurons to return to a resting state after activation. Changes in AChE activity may result from exposure to certain insecticides, which act as cholinesterase inhibitors. Inhibitors of AChE are also used to treat certain conditions such as dementia.

The Acetylcholinesterase Activity Microplate Assay Kit provides a simple and direct procedure for measuring AChE levels in a variety of samples such as blood, serum, and plasma. In this assay, thiocholine produced by AChE, reacts with DTNB to form a colorimetric (412 nm) product (TNB), proportional to the AChE activity present.

KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Reaction Buffer	20 ml x 1	4 °C
Substrate	Powder x 1	4 °C, keep in dark
Dye Reagent	Powder x 1	4 °C, keep in dark
Standard	Powder x 1	4 °C
Positive Control	Powder x 1	-20 °C
Technical Manual	1 Manual	

Note:

Substrate: add 1 ml distilled water to dissolve before use; store at 4 °C for 1 month after reconstitution.

Dye Reagent: add 1 ml ethanol to dissolve before use; store at 4 °C for 1 week after reconstitution.

Standard: add 1 ml distilled water to dissolve before use; then 250 µl into 750 µl distilled water, the concentration will be 5 mmol/L; store at -20 °C for 1 month after reconstitution.

Positive Control: add 1 ml Assay Buffer to dissolve before use; store at -80 °C for a month after reconstitution.

MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 412 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice
9. Ethanol

SAMPLE PREPARATION

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for 5×10^6 cell or bacteria, sonicate (with power 20%, sonicate 3s, interval 10s, repeat 30 times) ; centrifuged at 4000g 4 °C for 20 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 4000g 4 °C for 20 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

3. For serum or plasma samples

Detect directly.

ASSAY PROCEDURE

Warm Reaction Buffer to room temperature before use.

Add following reagents into the microplate:

Reagent	Sample	Control	Standard	Blank	Positive Control
Reaction Buffer	170 µl	170 µl	170 µl	170 µl	170 µl
Substrate	10 µl	10 µl	--	--	10 µl
Sample	10 µl	--	--	--	--
Distilled water	--	10 µl	10 µl	20 µl	--
Standard	--	--	10 µl	--	--
Positive Control	--	--	--	--	10 µl
Dye Reagent	10 µl	10 µl	10 µl	10 µl	10 µl

Mix, wait for 2 minutes, record absorbance measured at 412 nm.

Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range. If the enzyme activity is lower, please add more sample into the reaction system; or increase the reaction time; if the enzyme activity is higher, please dilute the sample, or decrease the reaction time.

CALCULATION

Unit Definition: One unit of AChE activity is defined as the enzyme hydrolyze 1 μ mol of Acetylthiocholine iodide per minute at 25°C and pH 7.4.

1. According to the protein concentration of sample

$$\begin{aligned} \text{AChE (U/mg)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (C_{\text{Protein}} \times V_{\text{Sample}}) / T \\ &= 2.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}} \end{aligned}$$

2. According to the weight of sample

$$\begin{aligned} \text{AChE (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times W / V_{\text{Assay}}) / T \\ &= 2.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

3. According to the quantity of cells or bacteria

$$\begin{aligned} \text{AChE (U}/10^4) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times N / V_{\text{Assay}}) / T \\ &= 2.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N \end{aligned}$$

4. According to the volume of sample

$$\begin{aligned} \text{AChE (U/mg)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} / T \\ &= 2.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$

C_{Standard} : the concentration of standard, 5 mmol/L = 5 μ mol/ml;

C_{Protein} : the protein concentration, mg/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria, $N \times 10^4$;

V_{Standard} : the volume of the standard, 0.01 ml;


V_{Sample} : the volume of sample, 0.01 ml;

V_{Assay} : the volume of Assay buffer, 1 ml;


T: the reaction time, 2 minutes.

TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

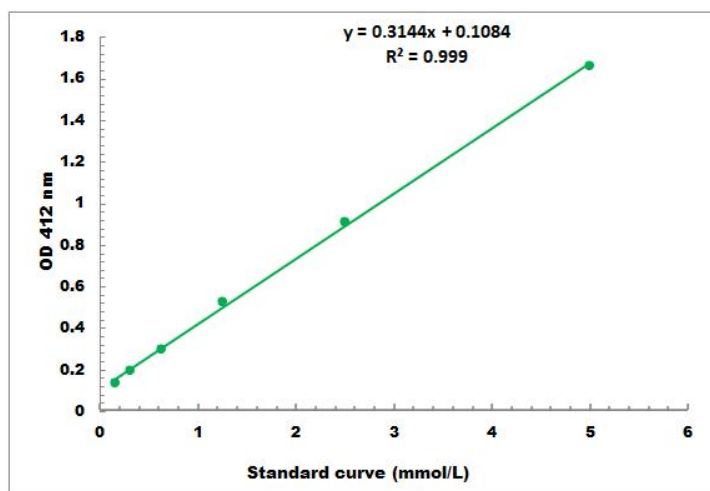

Detection Range: 0.1 mmol/L - 5 mmol/L

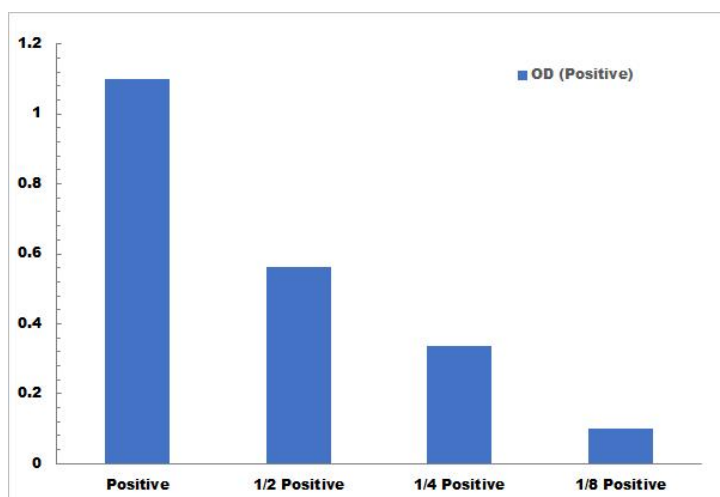

Positive Control reaction in 96-well plate assay with decreasing the concentration