

## Trypsin Microplate Assay Kit

**Cat #: orb390786 (manual)**

Detection and Quantification of Trypsin Activity in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and Other biological fluids Samples.

*For research use only. Not for diagnostic or therapeutic procedures.*

## INTRODUCTION

Trypsin (EC 3.4.21.4) is a serine protease found in the digestive system of many vertebrates, where it hydrolyses proteins. Trypsin is produced in the pancreas as the inactive proenzyme trypsinogen. Active trypsin predominantly cleaves peptide chains at the carboxyl side of the amino acids lysine or arginine, except when either is followed by proline. It is used for numerous biotechnological processes.

The assay is initiated with the enzymatic catalysis of the BAEE by Trypsin. The enzyme catalysed reaction products BA can be measured at a colorimetric readout at 253 nm.

**KIT COMPONENTS**

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Reaction Buffer	10 ml x 1	4 °C
Substrate	Powder x 1	4 °C
Substrate Diluent	1.2 ml x 1	RT
Stop Solution	10 ml x 1	4 °C
Standard (500 µmol/L)	1 ml x 1	4 °C
Positive Control	Powder x 1	-20 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

**Note:**

**Substrate:** add 1 ml Substrate Diluent to dissolve before use.

**Positive Control:** add 1 ml Assay Buffer to dissolve before use, mix.

**MATERIALS REQUIRED BUT NOT PROVIDED**

1. Microplate reader to read absorbance at 405 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice

## SAMPLE PREPARATION

### 1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for  $5 \times 10^6$  cell or bacteria, sonicate (with power 20%, sonicate 3s, interval 10s, repeat 30 times); centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

### 2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

### 3. For serum or plasma samples

Detect directly.

**ASSAY PROCEDURE**

Warm all reagents to room temperature before use.

Add following reagents into the microplate:

Reagent	Sample	Standard	Positive Control	Blank
Reaction Buffer	80 $\mu$ l	--	80 $\mu$ l	100 $\mu$ l
Substrate	10 $\mu$ l	--	10 $\mu$ l	--
Sample	10 $\mu$ l	--	--	--
Positive Control	--	--	10 $\mu$ l	--
Mix, put it in the oven, 37 °C for 10 minutes.				
Standard	--	100 $\mu$ l	--	--
Stop Solution	100 $\mu$ l	100 $\mu$ l	100 $\mu$ l	100 $\mu$ l
Mix, record absorbance measured at 405 nm.				

**Note:**

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range. If the enzyme activity is lower, please add more sample into the reaction system; or increase the reaction time; if the enzyme activity is higher, please dilute the sample, or decrease the reaction time.

## CALCULATION

**Unit Definition:** One unit of Trypsin activity is defined as the enzyme generates 1  $\mu\text{mol}$  of p-nitrophenol per minute.

1. According to the protein concentration of sample

$$\begin{aligned} \text{Trypsin (U/mg)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (C_{\text{Protein}} \times V_{\text{Sample}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / C_{\text{Protein}} \end{aligned}$$

2. According to the weight of sample

$$\begin{aligned} \text{Trypsin (U/g)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times W / V_{\text{Assay}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W \end{aligned}$$

3. According to the quantity of cells or bacteria

$$\begin{aligned} \text{Trypsin (U}/10^4) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times N / V_{\text{Assay}}) / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / N \end{aligned}$$

4. According to the volume of liquid sample

$$\begin{aligned} \text{Trypsin (U/ml)} &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} / T \\ &= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Blank}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) \end{aligned}$$

$C_{\text{Standard}}$ : the concentration of Standard,  $500 \mu\text{mol/L} = 0.5 \mu\text{mol/ml}$ ;

$C_{\text{Protein}}$ : the protein concentration, mg/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria,  $N \times 10^4$ ;

$V_{\text{Standard}}$ : the volume of standard, 0.1 ml;


$V_{\text{Sample}}$ : the volume of sample, 0.01 ml;

$V_{\text{Assay}}$ : the volume of Assay buffer, 1 ml;


T: the reaction time, 10 minutes.

## TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

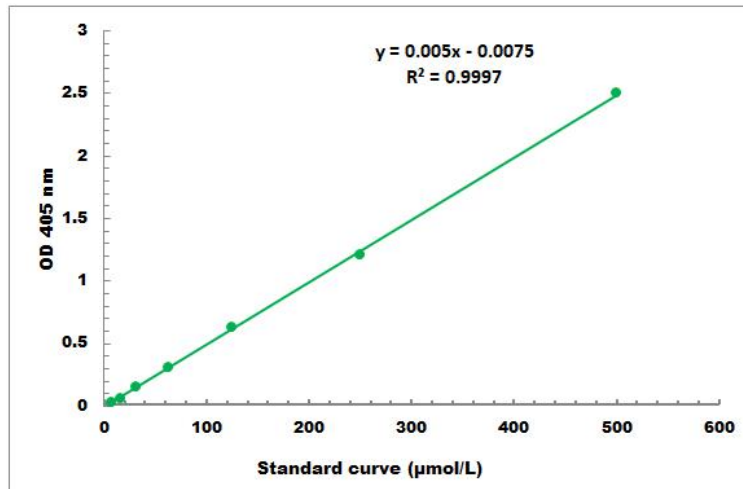

Detection Range: 5 µmol/L - 500 µmol/L

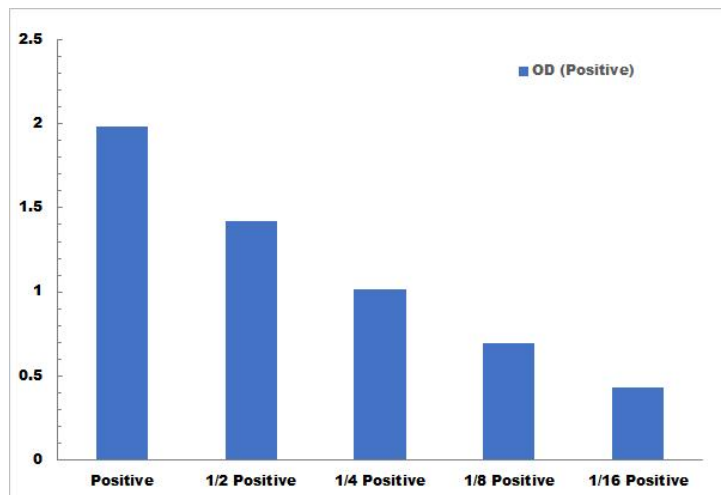

Positive Control reaction in 96-well plate assay with decreasing the concentration