

Maltose Microplate Assay Kit

Cat #: orb759231 (manual)

Detection and Quantification of Maltose Content in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media, Other biological fluids Samples.

For research use only. Not for diagnostic or therapeutic procedures.

INTRODUCTION

Maltose ($C_{12}H_{22}O_{11}$) is a disaccharide, composed of two glucose units linked by an α bond. It is produced from the hydrolysis of glycogen or starch, serving as a source of energy for plants and animals. Maltose can be found in foods such as grains, and other processed products.

Maltose Microplate Assay Kit provides a convenient means to measure maltose concentration in biological samples. In this assay, maltose is converted to two glucoses, which are then oxidized to form a colored product. The enzyme catalysated reaction products can be measured at a colorimetric readout at 540 nm.

KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Enzyme	Powder x 1	-20 °C
Reaction Buffer	12 ml x 1	4 °C
Dye Reagent	20 ml x 1	4 °C
Standard	Powder x 1	4 °C
Technical Manual	1 Manual	

Note:

Enzyme: add 1 ml reaction buffer to dissolve before use.

Standard: add 1 ml distilled water to dissolve before use, the concentration will be 5 mmol/L.

MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 540 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer

SAMPLE PREPARATION

1. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, put it in water bath of 80 °C for 10 minutes, centrifuged at 4, 000g at room temperature for 10 minutes, take the supernatant into a new centrifuge tube.

2. For liquid samples

Detect directly.

ASSAY PROCEDURE

Add following reagents into the microcentrifuge tubes:

Reagent	Sample	Control	Standard	Blank
Sample	40 μ l	40 μ l	--	--
Standard	--	--	40 μ l	--
Distilled water	--	--	--	40 μ l
Reaction Buffer	50 μ l	60 μ l	50 μ l	50 μ l
Enzyme	10 μ l	--	10 μ l	10 μ l
Mix, put it in the oven, 37 °C for 20 minutes.				
Dye Reagent	100 μ l	100 μ l	100 μ l	100 μ l
Mix, put it into the convection oven, 90 °C for 10 minutes, record absorbance measured at 540nm.				

Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) The concentrations can vary over a wide range depending on the different samples. For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range.

CALCULATION

1. According to the volume of sample

$$\begin{aligned}\text{Maltose } (\mu\text{mol/ml}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} \\ &= 5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}})\end{aligned}$$

2. According to the weight of sample

$$\begin{aligned}\text{Maltose } (\mu\text{mol/g}) &= (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / (V_{\text{Sample}} \times W / \\ &\quad V_{\text{Assay}}) \\ &= 5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / W\end{aligned}$$

C_{Standard} : the concentration of Standard, 5 mmol/L = 5 $\mu\text{mol/ml}$;

W: the weight of sample, g;


V_{Standard} : the volume of standard, 0.04 ml;

V_{Sample} : the volume of sample, 0.04 ml;

V_{Assay} : the volume of Assay buffer, 1 ml.

TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

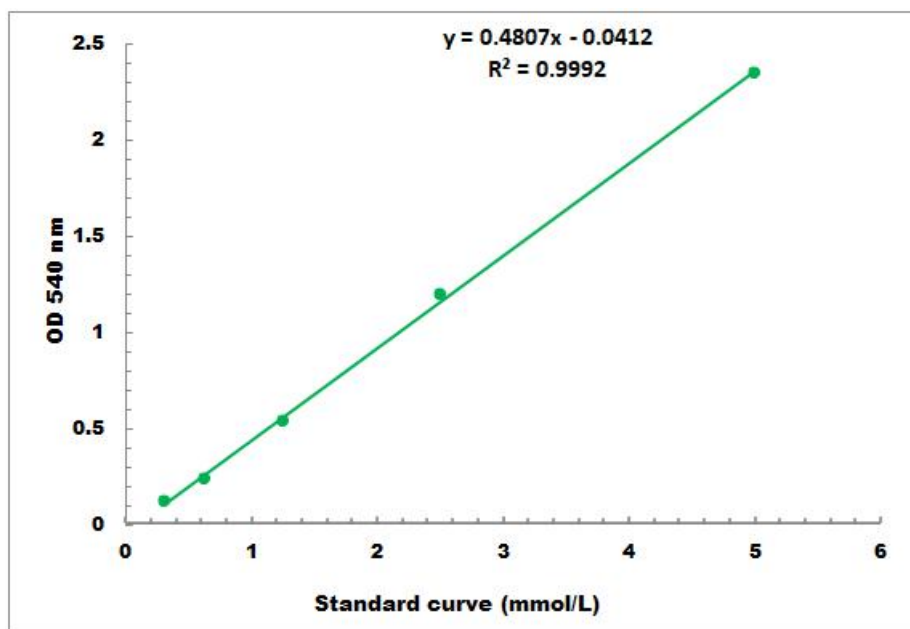

Detection Range: 0.5 mmol/L - 5 mmol/L