

Human PRG2 (Bone marrow proteoglycan) Quick ELISA Kit

Cat #: orb2568359 (manual)

Size: 48T/96T

For Research Use Only. Not For Use in Diagnostic Procedures!

Product Features

Application	In vitro quantitative determination of PRG2 concentrations in Serum, plasma, cell culture supernatant, cell lysate or tissue lysate, other biological fluid samples.		
Reactivity	Human	Detection Method	Sandwich ELISA, Double Antibody
Range	0.313-20ng/ml	Sensitivity	0.188ng/ml
Detection Duration	120 minutes (excluding balancing and sample preparation)		
Samples needed for single well(Max)	Serum: 50ul, Plasma: 50ul, Cell Culture Supernatant: 50ul, cell or tissue lysate: 50ul, Other liquid samples: 50ul		
Specificity	Specifically recognize PRG2, no obvious cross reaction with other analogues		
Storage	2-8°C (for sealed box), please do not freeze!		

Principle of the Assay

This kit was based on sandwich ELISA method. The experiment lasted 120 minutes. Capture antibody was conjugated to an affinity tag that was recognized by a specific antibody coated on the QuickTest plate. Add the Cap/ Det Ab working solution into each well, then add the standards and pilot samples into individual wells. If the sample contains PRG2, a capture antibody-PRG2-biotin-detection antibody complex was formed. After incubation, unbound conjugates were removed by wash buffer. HRP-Streptavidin was added. After washing, TMB substrates were added to visualize HRP enzymatic reaction. TMB was catalyzed by HRP to produce a blue color product that turned yellow after adding a stop solution. Read the O.D. absorbance at 450nm in a microplate reader. The concentration of PRG2 in the sample was calculated by drawing a standard curve. The concentration of the target substance is proportional to the OD450 value.

Kit Components and Storage

The sealed kit can be stored at 2-8 °C. The storage condition for opened kit is specified in the table below:

Item	Size(48T)	Size(96T)	Storage Condition for Opened Kit
ELISA Microplate (Dismountable)	8×6	8×12	Put the rest strips into a sealed foil bag with the desiccant. Stored for 1 month at 2-8°C; Stored for 12 months at -20°C
Lyophilized Standard	1vial	2vials	Put the rest standards into a desiccant bag. Stored for 1 month at 2-8°C; Stored for 12 months at -20°C
Cap/Det Ab (Ready to use)	3ml	6ml	2-8°C (Avoid Direct Light)
HRP-Streptavidin (Ready to use, orange)	5ml	10ml	
TMB Substrate	5ml	10ml	
Sample Dilution Buffer (blue)	20ml	20ml	2-8°C
Stop Solution	5ml	5ml	
Wash Buffer (25X)	15ml	30ml	
Plate Sealer	3 pieces	5 pieces	
Product Description	1 copy	1 copy	

Note: The liquid reagent bottle contains slightly more reagent than indicated on the label. Use a micropipette to measure accurately.

Required Instruments and Reagents

1. Microplate reader (wavelength: 450nm)
2. 37°C incubator (When using a water bath incubator, ensure the internal air temperature is 35-38°C; When using the cell CO2 incubator, use a sealed bag to isolate the microplate)
3. Automated plate washer or multi-channel pipette/5ml pipettor (for manual washing purpose)
4. Precision single (0.5-10µL, 5-50µL, 20-200µL, 200-1000µL) and multi-channel pipette with disposable tips (calibration is required before use.)
5. Sterile tubes and Eppendorf tubes with disposable tips
6. Absorbent paper and loading slot
7. Deionized or distilled water

Sample Collection and Storage

1. Serum

Place whole blood sample at room temperature for 2 hours or at 2-8°C overnight. Centrifuge for 20min at 1000xg and collect the supernatant to detect immediately. Or you can aliquot the supernatant and store it at -20°C or -80°C for future's assay.

2. Plasma

EDTA-Na₂/K₂ is recommended as the anticoagulant. Centrifuge samples for 15 minutes at 1000xg 2-8°C within 30 minutes after collection. Collect the supernatant to detect immediately. Or you can aliquot the supernatant and store it at -20°C or -80°C for future's assay. For other anticoagulant types and uses, please refer to the sample preparation guideline.

3. Tissue Sample

Generally, tissue samples are required to be made into homogenization. Protocol is as below:

3.1. Place the target tissue on the ice. Remove residual blood by washing tissue with pre-cooling PBS buffer (0.01M, pH=7.4). Then weigh for usage.

3.2. Use lysate to grind tissue homogenates on the ice. The adding volume of lysate depends on the weight of the tissue. Usually, 9mL PBS would be appropriate to 1 gram tissue pieces. Some protease inhibitors are recommended to add into the PBS (e.g. 1mM PMSF).

3.3. Do further process using ultrasonic disruption or freeze-thaw cycles (Ice bath for cooling is required during ultrasonic disruption; Freeze-thaw cycles can be repeated twice.) to get the homogenates.

3.4. Homogenates are then centrifuged for 5 minutes at 5000xg. Collect the supernatant to detect immediately. Or you can aliquot the supernatant and store it at -20°C or -80°C for future's assay.

3.5. Determine total protein concentration by BCA kit for further data analysis. Usually, total protein concentration for Elisa assay should be within 1-3mg/ml. Some tissue samples such as liver, kidney, pancreas which containing a higher endogenous peroxidase concentration may react with TMB substrate causing false positivity. In that case, try to use 1% H₂O₂ for 15min inactivation and perform the assay again.

Notes: PBS buffer or the mild RIPA lysis can be used as lysates. While using RIPA lysis, make the PH=7.3.

Avoid using any reagents containing NP-40 lysis buffer, Triton X-100 surfactant, or DTT due to their severe inhibition for kits' working. We recommend using 50mM Tris+0.9%NaCL+0.1%SDS, PH7.3. You can prepare by yourself or contact us for purchasing.

4. Cell Culture Supernatant

Collect the supernatant: Centrifuge at 2500 rpm at 2-8°C for 5 minutes, then collect clarified cell culture supernatant to detect immediately. Or you can aliquot the supernatant and store it at -80°C for future's assay.

5. Cell Lysate

5.1. Suspension Cell Lysate: Centrifuge at 2500 rpm at 2-8°C for 5 minutes and collect cells. Then add pre-cooling PBS into collected cell and mix gently. Recollect cell by repeating centrifugation. Add 0.5-1ml cell lysate and appropriate protease inhibitor (e.g. PMSF, working concentration: 1mmol/L). Lyse the cell on ice for 30min-1h or disrupt the cell by ultrasonic disruption.

5.2. Adherent Cell Lysate: Absorb supernatant and add pre-cooling PBS to wash three times. Add 0.5-1ml cell lysate and appropriate protease inhibitor (e.g. PMSF, working concentration: 1mmol/L). Scrape the adherent cell with cell scraper. Lyse the cell suspension added in the centrifuge tube on ice for 30min-1h or disrupt the cell by ultrasonic disruption.

5.3. During lysate process, use the tip for pipetting or intermittently shake the centrifugal tube to completely lyse the protein. Mucilaginous product is DNA which can be disrupted by ultrasonic cell disruptor on ice. (3~5mm probe, 150-300W, 3~5 s/time, 30s intervals for 1~2s working).

5.4. At the end of lysate or ultrasonic disruption, centrifuge at 10000rpm at 2-8°C for 10 minutes. Then, the supernatant is added into EP tube to detect immediately. Or you can aliquot the supernatant and store it at -80°C for future's assay.

Notes: Read notes in tissue sample. Determine total protein concentration by BCA kit for further data analysis. Usually, total protein concentration for Elisa assay should be within 1-3mg/ml.

6. Other Biological Sample

Centrifuge samples for 15 minutes at 1000×g at 2-8°C. Collect the supernatant to detect immediately. Or you can aliquot the supernatant and store it at -80°C for future's assay.

Recommended reagents for sample preparation: 100mM PMSF protease inhibitor, Lysis Buffer (for ELISA).

Notes for Samples

1. Blood collection tubes should be disposable and non-endotoxin. Avoid using hemolyzed and lipemia samples.
2. The best sample storage condition: less than 5 days at 2-8°C; within 6 months at -20°C; within 2 years at -80°C. Stored in liquid nitrogen for a longer storage. When melting frozen samples, rapid water bath at 15 - 25°C can decrease the effect of ice crystal (0°C) on the sample. After melting, centrifuge to remove the precipitate, and then mix well.
3. The detection range of this kit is not equivalent to the concentration of analyze in the sample. For analyses with higher or lower concentration, please properly dilute or concentrate the sample.
4. Pretest is recommended for special samples without reference data to validate the validity.
5. Recombinant protein may not match with the capture or detection antibody in the kit, resulting in the undetectable assay.

Precautions for Kits

1. When using different Elisa kits, labeling is required to avoid mixed components and failed assay.
2. After opening the kit, please refer to the table of storage condition for coated plate and standards (Dampness may decrease the activity.). If any component is missing or damaged during the assay or storage, please contact us for ordering a new one to replace.
3. Sterile and disposable tips are required during the assay. After use, the reagents bottle cap has to be tightened to avoid the microbial contamination and evaporation.
4. While manual washing, please keep tips or pipettors for adding wash buffer away from the well. Insufficient washing or contamination easily causes false positive and high background.

5. During the assay, prepare required reagents for next step in advance. After washing, add the reagent into the well in time to avoid dryness. Otherwise, dry plate will result in the failed assay.
6. Before confirmation, reagents from other batches or sources should not be used in this kit.
7. Don't reuse tips and tubes to avoid cross contamination.
8. After loading, seal the plate to avoid the evaporation of the sample during incubation. Complete the incubation process at recommended temperature.
9. Please wear the lab coat, mask and gloves to protect yourself during the assay. Especially, for the detection of blood or other body fluid samples, please follow regulations on safety protection of biological laboratory.

Recommended Sample Dilution Ratio

Please refer to shipped manuals or contact us for samples, dilution as well background info.

When the concentration of the target in sample is very low, the sample can be added directly without dilution.

If other dilution ratio for your sample model is required, please refer to the universal dilution ratio below. (The ratio is suitable for single-well assay. For duplicate assay, please follow the calculation: volume of sample and diluent x number of duplicate well)

For 2-fold dilution (1/2): One step dilution. Add 60ul sample into 60ul sample diluent and mix gently.

For 5-fold dilution (1/5): One step dilution. Add 24ul sample into 96ul sample diluent and mix gently.

For 10-fold dilution (1/10): One step dilution. Add 12ul sample into 108ul sample diluent and mix gently.

For 20-fold dilution (1/20): One step dilution. Add 6ul sample into 114ul sample diluent and mix gently.

For 50-fold dilution (1/50): One step dilution. Add 3ul sample and 47ul normal saline (0.9% NaCl) into 100ul sample diluent and mix gently.

For 100-fold dilution (1/100): One step dilution. Add 3ul sample and 177ul normal saline into 120ul sample diluent and mix gently.

For 1000-fold dilution (1/1000): Two step dilution. Create a 50-fold dilution first (normal saline is used throughout the dilution). Then, create a 20-fold dilution and mix gently.

For 10000-fold dilution (1/10000): Two step dilution. Create a 100-fold dilution first (normal saline is used throughout the dilution). Then, create the same dilution again and mix gently.

For 100000-fold dilution (1/100000): Three step dilution. Create a 50-fold dilution and 20-fold dilution respectively (normal saline is used in the first two steps.) Finally, create a 100-fold dilution and mix gently.

Notes: The volume in each dilution is not less than 3ul. Dilution factor should be within 100-fold. Mixing during dilution is required to avoid foaming

Reagent Preparation and Storage

Take the ELISA kit from the fridge around 20 minutes earlier and equilibrate to room temperature (18-25°C). For repeated assays, please just take the strips and standards required for the current assay, store the rest materials according to the relevant condition.

1. Wash Buffer

Dilute 30ml (15ml for 48T) concentrated wash buffer to 750ml (375ml for 48T) wash buffer with deionized or distilled water and mix well. (The recommended resistivity of ultrapure water is 18MΩ.) Alternatively, take appropriate amount of concentrated wash buffer according to the assay requirement, then create a 25-fold dilution and mix well. Store the rest solution at 2-8°C.

Crystals formed in the concentrated wash buffer can be heated by water bath at 40°C till complete dissolution. (Heating temperature should be below 50°C.) Mix well for the next step. It's better to use up the prepared wash buffer in one day. Store the rest buffer at 2-8°C within 48h.

2. Sample dilution

2.1. The "Recommended Sample Dilution Ratio" in the manual refers to the recommended dilution ratio for limited samples like normal serum, normal plasma, cell lysate or cell culture supernatant, not indicating the proteins' expression status in all the samples. Due to disease or model process, the optimal dilution ratio of your samples may be different from the recommended dilution ratio in the manual. To avoid experimental failure caused by unsuitable sample dilution ratio, it is recommended to carry out pre-experiment before formal assay, by selecting a small amount of samples from different groups and considering the "Recommended Sample Dilution ratio" and the corresponding disease or model treatment, setting 3 to 4 groups with 10-fold dilution to get the optimal dilution ratio. For example, target protein A in normal serum needs to be diluted at 1/100 and the disease will lead to its decrease, then you can set four gradients (1/10, 1/100, 1/1000, and 1/10000) while pre-experiment.

2.2. Please refer to "Recommended Sample Dilution Ratio" in the manual to learn operations in detail.


3. Standards

3.1. Centrifuge standards tube for 1min at 10000xg. Label it as Zero tube.

3.2. Add **0.5ml** sample dilution buffer into the standard tube. Tighten the tube cap and let it stand for 2min at room temperature. Invert the tube several times to mix gently. (Or you can mix it using a low-speed vortex mixer for 3-5 seconds.)

3.3. Centrifuge the tubes for 1min at 1000xg, making the liquid towards the bottom of tube and removing possible bubbles.

3.4. Standard dilution: Label 7 EP tubes with 1/2, 1/4, 1/8, 1/16, 1/32, 1/64 and blank respectively. Add 150ul of the sample dilution buffer into each tube. Add 150ul solution from zero tube into 1/2 tube and mix them thoroughly. Transfer 150ul from 1/2 tube into 1/4 tube and mix them thoroughly. Transfer 150ul from 1/4 tube into 1/8 tube and mix them thoroughly, so on till 1/64 tube. Now blank tube only contains 150ul sample dilution buffer. The standard concentration from zero tube to blank tube is 2X 20ng/ml, 20ng/ml, 10ng/ml, 5ng/ml, 2.5ng/ml, 1.25ng/ml, 0.625ng/ml, 0ng/ml.

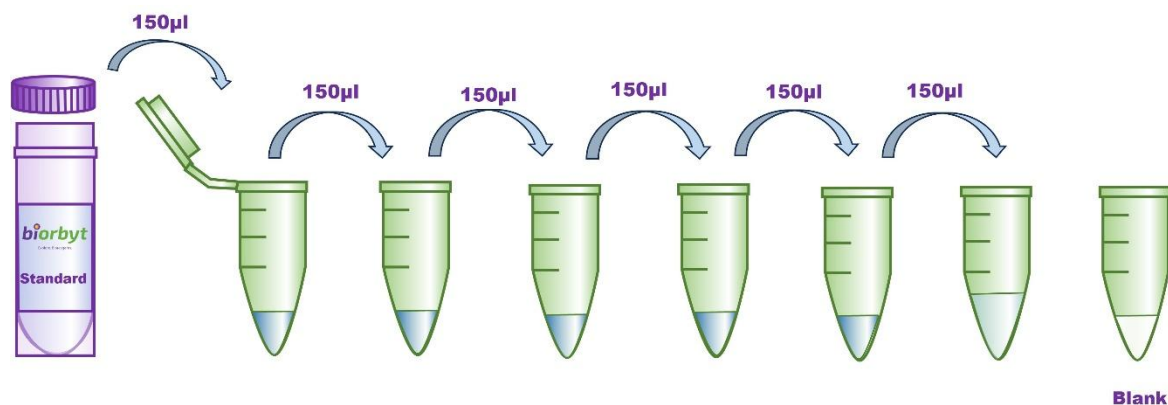

Notes: Store the zero tube with dissolved standards at 2-8°C and use it within 24h (Do not freeze). Other diluted working solutions containing standards should be used in 2h.

Assay Procedure Summary

Step 1: Take out the required plate wells, add 50ul Cap/Det Ab into each well, then add 50ul Standard or Sample into individual well. (When adding standard or sample, the disposable tip lightly touches the liquid level. Change the disposable tips for different samples and standards.) Gently tap the plate for 10s to ensure thorough mixing then static incubate for 60 minutes at 37°C.

Washing: Wash the plate twice without immersion.

Step 2: Add 100ul HRP-Streptavidin (orange) into each well, seal the plate and static incubate for 30 minutes at 37°C.

Washing: Wash the plate five times without immersion.

Step 3: Add 90ul TMB substrate solution, seal the plate and static incubate for 10-20 minutes at 37°C. (Accurate TMB visualization control is required.)

Step 4: Add 50ul stop solution. Read at 450nm immediately and calculate.

Detailed Assay Procedure

(It is necessary to continuously finish the whole experimental process. The reaction wells need to be immediately added with the working solution, which cannot be too dry. Otherwise, it might not work properly.)

When diluting samples, they must be mixed completely. It's recommended to plot a standard curve for each test.

1. Set standard, pilot samples, control (blank) wells on the pre-coated plate respectively, and then, records their positions. It's recommended to measure each standard and sample in duplicate to decrease experimental errors.
2. Cap/Det Ab and Standards/sample loading: Add 50ul Cap/Det Ab into each well. Aliquot 50ul of zero tube, 1/2 tube, 1/4 tube, 1/8 tube, 1/16 tube, 1/32 tube, 1/64 tube and blank into each standard well. Then, add 50ul pilot samples into sample wells. Immediately, gently tap the plate for 10s to ensure thorough mixing then static incubate for 60 minutes at 37°C. (When adding standard or sample, the disposable tip lightly touches the liquid level. Change the disposable tips for different samples and standards.)

Explore. Bioreagents.

3. Wash twice: Remove the cover, then absorb the liquid in the plate or tap the plate on a clean absorbent paper two or three times. Add 300-350ul wash buffer into each well without immersion. Discard the liquid in the well and tap on the absorbent paper again. Repeat the washing step twice.
4. HRP-Streptavidin: Add 100ul HRP-Streptavidin into each well. Seal the plate and static incubate for 30 minutes at 37°C. (Put the whole bottle of TMB into room temperature for 30min.)
5. Wash five times: Remove the cover, and then wash the plate with wash buffer five times. Read washing method in step 3.
6. TMB Substrate: Add 90ul TMB Substrate into each well, seal the plate and static incubate at 37°C in dark within 10-20 minutes. Run the microplate reader and preheat for 15min. (Notes: Please do not use the reagent reservoirs used by HRP couplings. The reaction time can be shortened or extended according to the actual color change, but not more than 30 minutes. You can terminate the reaction when apparent gradient appeared in standard wells. Weaker or stronger color intensity is unacceptable.)
7. Stop: Keep the liquid in the well after staining. Add 50ul stop solution into each well. The color will turn yellow immediately. The order for adding stop solution and TMB substrate solution is the same.
8. OD Measurement: Read the O.D. absorbance at 450nm in a microplate reader immediately. (If your microplate reader has a choice of correction wavelength, set it to 570nm or 630nm. Correct the read value to the OD450 value minus the OD570 or OD630 value. In this way, the OD value of non-chromogenic substances can be corrected and removed, thus obtaining more accurate results. If the microplate reader does not have a 570nm or 630nm wavelength, the original OD450 value can be used.)

Calculation of Results

1. Calculate the mean OD450 value (using the original OD450 value or the corrected OD450 value) of the duplicate readings for each standard, control, and sample. Then, obtain the value of calculation by subtracting the OD450 blank.
2. Create a four-parameter logistic curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis. (Remove the OD450 blank during plotting.) Alternatively, you can use the curve fitting software offered by the microplate reader (e.g. Thermo SkanIt RE software, Curve Expert 1.3 or 1.4).
3. Calculate the sample concentration by substituting OD450 value into the standard curve.


Note: If the sample is added undiluted, the sample dilution caused by incubation of both the sample and antibody should be considered. In this case, the final concentration should be multiplied by 2 from the calculated value. If the sample is 1/100 diluted before adding the plate wells, the final concentration should be multiplied by 200 from the calculated value. And so on.

Typical Data & Standard Curve

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual. (The humidity in the laboratory is 20%-60%, and the temperature is 18°C -25°C. (TMB was balanced to room temperature before color development, and incubated at 37°C for 15 minutes in the dark after adding the enzyme label plate holes.)

The following assay data are provided for reference, since experimental environment and operation are different. The establishment of standard curve depends on your own assay.

STD.(ng/ml)	OD-1	OD-2	Average	Corrected
0	0.077	0.079	0.078	0
0.312	0.134	0.132	0.133	0.055
0.625	0.192	0.188	0.19	0.112
1.25	0.375	0.372	0.359	0.281
2.5	0.65	0.644	0.616	0.538
5	0.977	0.985	1.005	0.927
10	1.678	1.693	1.649	1.571
20	2.339	2.283	2.3	2.222

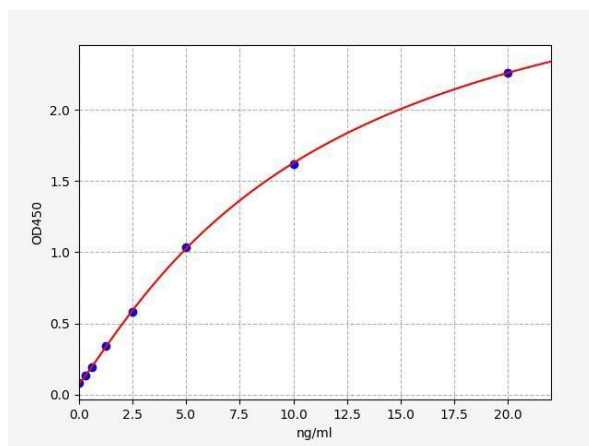

Precision

Intra-assay Precision: samples with low, medium and high concentration are tested 20 times on same plate.

Inter-assay Precision: samples with low, medium and high concentration are tested 20 times on three different plates.

Item	Intra-assay Precision			Inter-assay Precision		
	1	2	3	1	2	3
Sample	1	2	3	1	2	3
n	20	20	20	20	20	20
Mean (ng/ml)	0.59	2.42	10.01	0.6	2.54	9.94
Standard deviation	0.02	0.09	0.42	0.02	0.11	0.43
CV(%)	4.1	3.56	4.23	3.47	4.49	4.37

Recovery

Add a certain amount of PRG2 into the sample. Calculate the recovery by comparing the measured value with the expected amount of PRG2 in the sample.

Matrix	Recovery Range (%)	Average (%)
Serum(n=5)	90-102	96
EDTA Plasma(n=5)	85-100	95
Heparin Plasma(n=5)	83-105	93

Linearity

Dilute the sample with a certain amount of PRG2 at 1:2, 1:4 and 1:8 to get the recovery range.

Sample	1:2	1:4	1:8
Serum(n=5)	89-105%	97-104%	92-102%
EDTA Plasma(n=5)	85-98%	83-94%	83-98%
Heparin Plasma(n=5)	81-87%	82-99%	82-97%

Stability

Perform the stability test for the sealed kit at 37°C and 2-8°C and get relevant data.

ELISA kit(n=5)	37°C for 1 month	2-8°C for 6 months	2-8°C for 12 months
Average (%)	80	95-100	85-98

ELISA Troubleshooting

High background/non-specific staining

Description of results	Possible reason	Recommendations and precautions
After stopping the reaction, the entire plate shows a uniform yellow or light color, or the standard curve is linear but the background signal is excessively high.	Yellowing of the entire plate may be caused by incorrect addition of reagents.	Before starting the experiment, verify the components and lot numbers of all reagents to ensure they belong to the same kit. Reagents from different kits or different lot numbers must not be mixed.
	The ELISA plate was not washed sufficiently.	Ensure that the same volume of Wash Solution is added to each microwell during the washing process. After washing, firmly tap the ELISA plate on absorbent paper to remove any residual buffer.
	Incubation time was too long.	Strictly follow the procedures outlined in the manual.
	Streptavidin-HRP contaminated the pipette tip or TMB container, or the positive control contaminated the pre-coated microplate.	Replace pipette tips when dispensing different reagents. Use separate containers when preparing different reagent components, and always use a pipette during handling.
	The concentration of Biotinylated Antibody or Streptavidin-HRP was too high.	Verify that concentration calculations are correct, or perform further dilution if necessary.
	The substrate was exposed to light or contaminated prior to use.	Store reagents in the dark at all times prior to substrate addition.
	Color development time was too long.	Strictly follow the procedures outlined in the manual.
	An incorrect filter was used when reading the absorbance value.	When TMB is used as the substrate, measure absorbance at 450 nm.

NO color plates

Description of results	Possible reason	Recommendations and precautions
After the color development step, all wells of the ELISA plate are	Components from different reagent sets were mixed.	Carefully read reagent labels when preparing or using them.

colorless, and the positive control is not clearly detectable. s	During plate washing or sample/enzyme addition, the enzyme label was contaminated or inactivated, resulting in loss of its ability to catalyze color development.	Confirm that the container holding the ELISA plate does not contain enzyme inhibitors (such as NaN_3), and ensure that the container used to prepare the Wash Solution has been thoroughly cleaned.
	A reagent or procedural step was omitted.	Review the manual carefully and strictly follow the operating procedures.

Light color

Description of results	Possible reason	Recommendations and precautions
The Standard appears normal, but the sample color is weak.	The sample contains NaN_3 preservative, which inhibits the enzyme reaction.	Samples must not contain NaN_3 .
	The sample being tested may not contain strongly positive material, so the result may be normal.	If there is any doubt about the results, repeat the assay.
The visual result appears normal, but the microplate reader values are low.	An incorrect filter was used for absorbance measurement.	When TMB is used as the substrate, absorbance should be measured at 450 nm.
All wells, including Standards and Samples, show weak color development.	Insufficient incubation time.	Ensure accurate timing using a timer.
	Inadequate color development.	Typically 15–30 minutes.
	Excessive washing, or the dilution ratio of the concentrated Wash Buffer does not meet requirements.	Minimize the impact of washing by diluting the concentrated Wash Buffer and setting the washing time according to the manual. Accurately record the number of washes and the volume used.
	Poor quality distilled water.	The prepared Wash Buffer should be tested to confirm that the pH is neutral.
	During plate washing or sample addition, the enzyme label was contaminated or inactivated, resulting in loss of catalytic activity.	Confirm that the container holding the ELISA plate does not contain enzyme inhibitors (such as NaN_3), that the container used to prepare the Wash Buffer has been thoroughly cleaned, and that the purified water used meets the required standards and is not contaminated.
	The kit has expired or was improperly stored.	Use the kit within its expiration date and store it according to the conditions recommended in the manual to avoid contamination.

	Reagents and samples were not equilibrated to room temperature before use.	Allow all reagents and samples to equilibrate at room temperature for approximately 30 minutes before use.
	Insufficient pipetting volume, overly rapid dispensing, excessive liquid remaining on the inner wall of the tip, or unclean tip walls.	Calibrate the pipette properly. Ensure tips are compatible and fit securely, pipette at an appropriate speed, and fully dispense the liquid. Tips should have clean inner walls and be used only once
Poor repeatability.	Incubation temperature was not properly controlled.	Maintain a constant incubation temperature and avoid localized temperature extremes.
	Excess liquid remained on the inner wall of the wells during liquid addition.	When adding liquids, dispense along the lower inner wall of the wells without touching the bottom.
	Reuse of consumables.	Replace pipette tips when drawing different reagents, and use separate containers when preparing different reagent components.
	The bottom of the microwell is scratched or contaminated.	Handle the plate carefully. Avoid touching the well bottoms and clean the bottom of the microplate to remove dirt or fingerprints. Perform technical replicates of the same sample three times, ensuring that at least two values are comparable.
	Cross-contamination during sample addition.	Minimize the risk of cross-contamination during sample addition.
The color development across the plate is uneven and irregular.	Cross-contamination during manual plate washing.	When washing plates manually, discard the first three washes immediately, then allow soaking during subsequent washes to reduce cross-contamination.
	Cross-contamination during plate tapping.	Use appropriate absorbent paper when tapping the plate. Avoid introducing foreign material into the wells, and avoid tapping in the same position repeatedly to reduce cross-contamination.

Description of results	Possible reason	Recommendations and precautions
The color development of the plate is uneven and irregular	The liquid dispensing head of the plate washer is clogged, leading to improper liquid dispensing or excessive residual liquid after aspiration, which results in uneven and irregular color development across the plate.	Unclog the liquid dispensing head to ensure that each well is properly filled with wash solution during plate washing and that minimal residual liquid remains after aspiration.

Incomplete centrifugation of the sample, resulting in coagulation within the reaction wells or interference from sediment or residual cellular components.	Serum and plasma samples should be fully centrifuged at 3000 rpm for more than 6 minutes.
The sample was stored for an excessively long period, leading to contamination.	Samples should be kept fresh or stored at low temperatures to prevent contamination.
Incorrect preparation of the Wash Solution or direct use of the concentrated Wash Solution.	Prepare all reagents strictly according to the manual.

Declaration

1. Limited to current conditions and scientific techniques, all raw materials are not completely identified and analyzed. This product may have a technology-related quality risk.
2. During the ELISA kit development, some endogenous interferons (not all) in the biological sample have been removed or decreased.
3. The final assay result is related to the validity of reagents, experimental operation and environment. Biorbyt is only responsible for this kit, excluding sample consumption during using this kit. Before use, please consider and prepare enough samples required by the assay.
4. To get a satisfied assay result, please use all reagents offered by this kit. Don't use any product from other vendors. Strictly follow instructions of this manual.
5. During assay procedure, incorrect reagents preparation and parameter setting of the microplate reader may result in the abnormal result. Before assay, please read this manual carefully and adjust instruments.
6. Even if the assay is performed by the same person, results in two independent assays may be different. Thus, each step in the assay should be controlled to ensure the reproducibility.
7. Before delivery, this kit is subject to the strict QC. Influenced by transportation conditions and experimental devices, the assay result got by the customer may be different from original data. Inter-assay CV between different batches may be caused by reasons before.
8. This kit is not compared to similar kits from other vendors or methods for testing the same detection target. Thus, assay results may be inconsistent.
9. This kit allows for research use only. For IVD or other purposes, Biorbyt is not responsible for relevant consequences and doesn't bear any legal liability.