

Thioredoxin Reductase Microplate Assay Kit

Cat #: orb390748 (manual)

For Research Use Only. Not For Use in Diagnostic Procedures!

Detection and Quantification of Thioredoxin Reductase (TrxR) Activity in Urine, Serum, Plasma, Tissue extracts, Cell lysate, Cell culture media and Other biological fluids Samples.

INTRODUCTION

Thioredoxin reductase (TrxR) (EC 1.8.1.9) is a ubiquitous enzyme which is involved in many cellular processes such as cell growth, p53 activity, and protection against oxidation stress, etc. The mammalian TrxR reduces thioredoxins as well as non-disulfide substrates such as selenite, lipoic acids, lipid hydroperoxides, and hydrogen peroxide.

Thioredoxin Reductase Microplate Assay Kit provides a convenient colorimetric assay for detecting TrxR activity in various samples. In the assay TrxR catalyzes the reduction of 5, 5'-dithiobis (2-nitrobenzoic) acid (DTNB) with NADPH to 5-thio-2-nitrobenzoic acid (TNB²⁻), which generate a strong yellow color ($\lambda_{\text{max}} = 450 \text{ nm}$).

KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Assay Buffer	30 ml x 4	4 °C
Reaction Buffer	20 ml x 1	4 °C
Substrate	Powder x 1	-20 °C
Dye Reagent	Powder x 1	4 °C
Dye Reagent Diluent	10 ml x 1	4 °C
Standard	Powder x 1	-20 °C
Positive Control	Powder x 1	-20 °C
Technical Manual	1 Manual	

Note:

Substrate: add 8 ml Reaction Buffer to dissolve before use; store at -80 °C for a month after reconstitution.

Dye Reagent: add 10 ml PBS to dissolve before use; store at -20°C for a month. **Standard:** add 1 ml distilled water to dissolve, mix; the concentration will be 5 mmol/L; store at -20°C for a month.

Positive Control: add 0.1 ml Assay Buffer to dissolve before use; store at -80 °C for a month after reconstitution.

MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 450 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice

SAMPLE PREPARATION

1. For cell and bacteria samples

Collect cell or bacteria into centrifuge tube, discard the supernatant after centrifugation, add 1 ml Assay buffer for 5×10^6 cell or bacteria, sonicate (with power 20%, sonicate 3s, interval 10s, repeat 30 times); centrifuged at 8,000g 4 °C for 10 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

2. For tissue samples

Weigh out 0.1 g tissue, homogenize with 1 ml Assay buffer on ice, centrifuged at 8,000g 4 °C for 20 minutes, take the supernatant into a new centrifuge tube and keep it on ice for detection.

3. For serum or plasma samples Detect directly.

ASSAY PROCEDURE

Warm the Assay Buffer to room temperature before use. Add following reagents in the microplate:

Reagent	Sample	Control	Standard	Blank	Positive Control
Substrate	80 µl	80 µl	--	--	80 µl
Reaction Buffer	--	20 µl	80 µl	80 µl	--
Sample	20 µl	--	--	--	--
Positive Control	--	--	--	--	20 µl
Standard	--	--	20 µl	--	--
Distilled water	--	--	100 µl	120 µl	--
Mix.					
Dye Reagent	100 µl	100 µl	--	--	100 µl
Mix, incubate at room temperature for 10 minutes, measured at 450 nm and record the absorbance.					

Note:

- 1) Perform 2-fold serial dilutions of the top standards to make the standard curve.
- 2) For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range. If the enzyme activity is lower, please add more sample into the reaction system; or increase the reaction time; if the enzyme activity is higher, please dilute the sample, or decrease the reaction time.
- 3) Reagents must be added step by step, cannot be mixed and added together.

CALCULATION

Unit Definition: One unit of TrxR activity is defined as the amount of enzyme which produces 1 µmol of TNB per minute at 37°C.

1. According to the protein concentration of sample

$$\text{TrxR (U/mg)} = (C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / (V_{\text{Sample}} \times C_{\text{Protein}}) / T$$

$$= 0.5 \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / C_{\text{Protein}}$$

2. According to the weight of sample

$$\text{TrxR (U/g)} = (C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / (W \times V_{\text{Sample}} / V_{\text{Assay}}) / T$$

$$= 0.5 \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / W$$

3. According to the quantity of cell or bacteria

$$\text{TrxR (U/10}^4\text{)} = (C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / (N \times V_{\text{Sample}} / V_{\text{Assay}}) / T$$

$$T = 0.5 \times (OD_{\text{Sample}} - OD_{\text{Control}}) / (OD_{\text{Standard}} - OD_{\text{Blank}}) / N$$

4. According to the volume of sample

$$\text{TrxR (U/ml)} = (C_{\text{Standard}} \times V_{\text{Standard}}) \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}}) / V_{\text{Sample}} / T$$

$$= 0.5 \times (\text{OD}_{\text{Sample}} - \text{OD}_{\text{Control}}) / (\text{OD}_{\text{Standard}} - \text{OD}_{\text{Blank}})$$

C_{Protein} : the protein concentration, mg/ml;

C_{Standard} : the concentration of standard, 5 mmol/L = 5 μ mol/ml;

W: the weight of sample, g;

N: the quantity of cell or bacteria, $N \times 10^4$;

V_{Sample} : the volume of sample, 0.02 ml;


V_{Standard} : the volume of standard, 0.02 ml;

V_{Assay} : the volume of Assay buffer, 1 ml;


T: the reaction time, 10 minutes.

TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

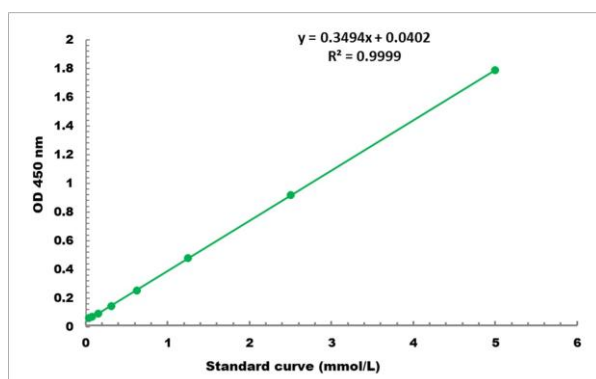

Detection Range: 0.05 mmol/L - 5 mmol/L

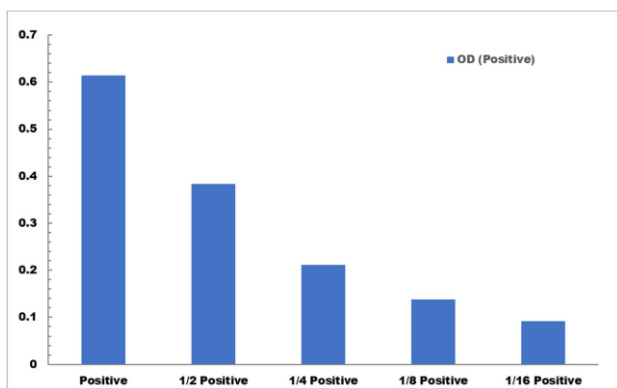

Positive Control reaction in 96-well plate assay with decreasing the concentration