



Human IL-20 ELISA Kit

Product Manual

Catalog No. orb99227



Tel: +44-1223-859-353 **Fax:** +44-1223-280-240
Email: info@biorbyt.com **VAT Nr.:** GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 **Fax:** +1-415-651-8558
Email: info@biorbyt.com **EIN:** 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



Introduction:


For quantitative detection of human IL-20 in cell culture supernates, serum and plasma(heparin, EDTA).

Typical Data Obtained from Human IL-20
(TMB reaction incubate at 37°C for 20 min)

Concentration(pg/ml)	0.0	62.5	125	250	500	1000	2000	4000
O.D	0.040	0.135	0.259	0.467	0.806	1.313	1.918	2.586

Typical Human IL-20 ELISA Kit Standard Curve

This standard curve was generated at Biorbyt for demonstration purpose only. A standard curve must be run with each assay.

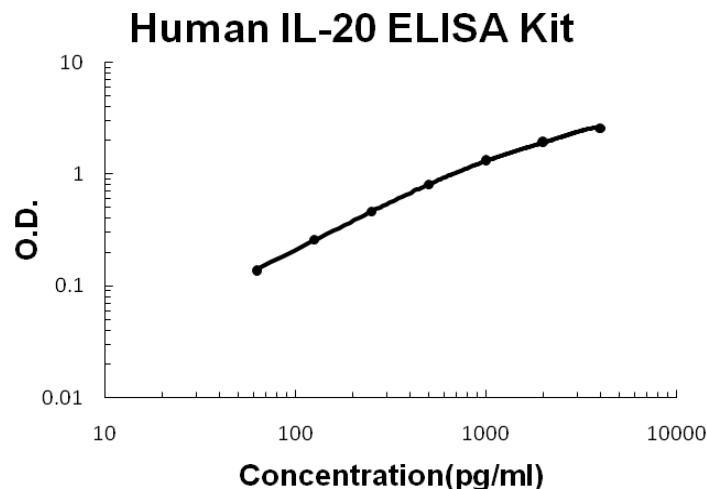

- Range** 62.5pg/ml-4000pg/ml
- Sensitivity** < 10pg/ml
- Specificity** Natural and recombinant human IL-20
- Cross-reactivity** No detectable cross-reactivity with other relevant proteins

Storage

Store at 4°C for 6 months, at -20°C for 12 months. Avoid multiple freeze-thaw cycles (Shipped with wet ice.)



Tel: +44-1223-859-353 **Fax:** +44-1223-280-240
Email: info@biorbyt.com **VAT Nr.:** GB 991815777
Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 **Fax:** +1-415-651-8558
Email: info@biorbyt.com **EIN:** 33-1226022
Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



Principle

Biorbyt's human IL-20 ELISA Kit was based on standard sandwich enzyme-linked immune-sorbent assay technology. A monoclonal antibody from mouse specific for IL-20 has been precoated onto 96-well plates. Standards(E.coli,L25-E176) and test samples are added to the wells, a biotinylated detection polyclonal antibody from goat specific for IL-20 is added subsequently and then followed by washing with PBS or TBS buffer. Avidin-Biotin-Peroxidase Complex was added and unbound conjugates were washed away with PBS or TBS buffer. HRP substrate TMB was used to visualize HRP enzymatic reaction. TMB was catalyzed by HRP to produce a blue color product that changed into yellow after adding acidic stop solution. The density of yellow is proportional to the human IL-20 amount of sample captured in plate.

Kit Components

Catalog number	Description	Quantity
-	96-well plate precoated with anti- human IL-20 antibody	1
orb97216	Lyophilized recombinant human IL-20 standard	10ng/tube×2
-	Biotinylated anti- human IL-20 antibody	130µl(dilution 1:100)
orb90540	Avidin-Biotin-Peroxidase Complex (ABC)	130µl(dilution 1:100)
orb90546	Sample diluent buffer	30 ml
orb90538	Antibody diluent buffer	12ml
orb90539	ABC diluent buffer	12ml
orb90526	TMB color developing agent	10ml
orb90523	TMB stop solution	10ml

Material Required But Not Provided

1. Microplate reader in standard size.
2. Automated plate washer.
3. Adjustable pipettes and pipette tips. Multichannel pipettes are recommended in the condition of large amount of samples in the detection.
4. Clean tubes and Eppendorf tubes.
5. Washing buffer (neutral PBS or TBS).

☒Preparation of 0.01M **TBS**: Add 1.2g Tris, 8.5g NaCl; 450µl of purified acetic acid or 700µl of concentrated

hydrochloric acid to 1000ml H₂O and adjust pH to 7.2-7.6. Finally, adjust the total volume to 1L.

☒Preparation of 0.01 M **PBS**: Add 8.5g sodium chloride, 1.4g Na₂HPO₄ and 0.2g NaH₂PO₄ to 1000ml distilled water and adjust pH to 7.2-7.6. Finally, adjust the total volume to 1L.



Tel: +44-1223-859-353 Fax: +44-1223-280-240
Email: info@biorbyt.com VAT Nr.: GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 Fax: +1-415-651-8558
Email: info@biorbyt.com EIN: 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



Notice for Application of Kit

1. To inspect the validity of experiment operation and the appropriateness of sample dilution proportion, pilot experiment using standards and a small number of samples is recommended.
2. The TMB Color Developing agent is colorless and transparent before using, contact us freely if it is not the case.
3. Before using the Kit, spin tubes and bring down all components to the bottom of tubes.
4. Duplicate well assay is recommended for both standard and sample testing.
5. Don't let 96-well plate dry, for dry plate will inactivate active components on plate.
6. Don't reuse tips and tubes to avoid cross contamination.
7. To avoid to use the reagents from different batches together.
8. In order to avoid marginal effect of plate incubation due to temperature difference (reaction may be stronger in the marginal wells), it is suggested that the diluted ABC and TMB solution will be pre-warmed in 37°C for 30 min before using.



Tel: +44-1223-859-353 **Fax:** +44-1223-280-240
Email: info@biorbyt.com **VAT Nr.:** GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 **Fax:** +1-415-651-8558
Email: info@biorbyt.com **EIN:** 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



Preparation

1. Sample Preparation and Storage

Store samples to be assayed within 24 hours at 2-8°C. For long-term storage, aliquot and freeze samples at -20°C. Avoid repeated freeze-thaw cycles.

- ☒ **Cell culture supernates:** Remove particulates by centrifugation, assay immediately or aliquot and store samples at -20°C.
- ☒ **Serum:** Allow the serum to clot in a serum separator tube (about 4 hours) at room temperature. Centrifuge at approximately 1000 X g for 15 min. Analyze the serum immediately or aliquot and store samples at -20°C.
- ☒ **Plasma:** Collect plasma using **heparin** or **EDTA** as an anticoagulant. Centrifuge for 15 min at 1500 x g within 30 min of collection. Assay immediately or aliquot and store samples at -20°C.

2. Sample Dilution Guideline

The user needs to estimate the concentration of the target protein in the sample and select a proper dilution factor so that the diluted target protein concentration falls near the middle of the linear regime in the standard curve. Dilute the sample using the provided diluent buffer. The following is a guideline for sample dilution. Several trials may be necessary in practice. **The sample must be well mixed with the diluents buffer.**

- ☒ **High target protein concentration (40-400ng/ml).** The working dilution is 1:100. i.e. Add 3 µl sample into 297 µl sample diluent buffer.
- ☒ **Medium target protein concentration (4-40ng/ml).** The working dilution is 1:10. i.e. Add 25 µl sample into 225 µl sample diluent buffer.
- ☒ **Low target protein concentration (62.5-4000pg/ml).** The working dilution is 1:2. i.e. Add 100 µl sample to 100 µl sample diluent buffer.
- ☒ **Very Low target protein concentration (≤62.5pg/ml).** No dilution necessary, or the working dilution is 1:2.

3. Reagent Preparation and Storage

- A. Reconstitution of the human IL-20 standard : IL-20 standard solution should be prepared no more than 2 hours prior to the experiment. Two tubes of IL-20 standard (10ng per tube) are included in



Tel: +44-1223-859-353 Fax: +44-1223-280-240
Email: info@biorbyt.com VAT Nr.: GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 Fax: +1-415-651-8558
Email: info@biorbyt.com EIN: 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



each kit. Use one tube for each experiment.

- a. 10,000pg/ml of human IL-20 standard solution: Add 1 ml sample diluent buffer into one tube, keep the tube at room temperature for 10 min and mix thoroughly.
- b. 4000pg/ml of human IL-20 standard solution: Add 0.4ml of the above 10ng/ml IL-20 standard solution into 0.6ml sample diluent buffer and mix thoroughly.
- c. 2000pg/ml→62.5pg/ml of human IL-20 standard solutions: Label 6 Eppendorf tubes with 2000pg/ml, 1000pg/ml, 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml respectively. Aliquot 0.3ml of the sample diluent buffer into each tube. Add 0.3ml of the above 4000pg/ml IL-20 standard solution into 1st tube and mix. Transfer 0.3 ml from 1st tube to 2nd tube and mix. Transfer 0.3ml from 2nd tube to 3rd tube and mix, and so on.

Note: The standard solutions are best used within 2 hours. The 10ng/ml standard solution should be stored at 4℃ for up to 12 hours, or at -20℃ for up to 48 hours. Avoid repeated freeze-thaw cycles.

- B. Preparation of biotinylated anti-human IL-20 antibody working solution: The solution should be prepared no more than 2 hours prior to the experiment.
- a. The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
 - b. Biotinylated anti-human IL-20 antibody should be diluted in 1:100 with the antibody diluent buffer and mixed thoroughly. (i.e. Add 1µl Biotinylated anti-human IL-20 antibody to 99µl antibody diluent buffer.)



Tel: +44-1223-859-353 Fax: +44-1223-280-240
Email: info@biorbyt.com VAT Nr.: GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 Fax: +1-415-651-8558
Email: info@biorbyt.com EIN: 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



- C. Preparation of Avidin-Biotin-Peroxidase Complex (ABC) working solution: The solution should be prepared no more than 1 hour prior to the experiment.
- The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
 - Avidin- Biotin-Peroxidase Complex (ABC) should be diluted in 1:100 with the ABC dilution buffer and mixed thoroughly. (i.e. Add 1µl ABC to 99µl ABC diluent buffer.)

Assay Procedure

The ABC working solution and TMB color developing agent must be kept warm at 37°C for 30 min before use. When diluting samples and reagents, they must be mixed completely and evenly. Standard IL-20 detection curve should be prepared for each experiment. The user will decide sample dilution fold by crude estimation of IL-20 amount in samples.

- Aliquot 0.1ml per well of the 4000pg/ml, 2000pg/ml, 1000pg/ml, 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml human IL-20 standard solutions into the precoated 96-well plate. Add 0.1ml of the sample diluent buffer into the control well (Zero well). Add 0.1ml of each properly diluted sample of human cell culture supernates, serum or plasma (heparin, EDTA) to each empty well. **See “Sample Dilution Guideline” above for details.** It is recommended that each human IL-20 standard solution and each sample be measured in duplicate.
- Seal the plate with the cover and incubate at 37°C for 90 min.
- Remove the cover, discard plate content, and blot the plate onto paper towels or other absorbent material. Do NOT let the wells completely dry at any time.
- Add 0.1ml of biotinylated anti-human IL-20 antibody working solution into each well and incubate the plate at 37°C for 60 min.
- Wash plate 3 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (**Plate Washing Method:** Discard the solution in the plate without touching the side walls. Blot the plate onto paper towels or other absorbent material. Soak each well with at least 0.3 ml PBS or TBS buffer for 1~2 minutes. Repeat this process two additional times for a total of THREE washes. Note: For automated washing, aspirate all wells and wash THREE times with PBS or TBS buffer, overfilling wells with PBS or TBS buffer. Blot the plate onto paper towels or other



Tel: +44-1223-859-353 Fax: +44-1223-280-240
Email: info@biorbyt.com VAT Nr.: GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 Fax: +1-415-651-8558
Email: info@biorbyt.com EIN: 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



absorbent material.)

6. Add 0.1ml of prepared ABC working solution into each well and incubate the plate at 37°C for 30 min.
7. Wash plate 5 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1-2 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (See Step 5 for plate washing method).
8. Add 90µl of prepared TMB color developing agent into each well and incubate plate at 37°C in dark for 20-25 min (**Note:** For reference only, the optimal incubation time should be determined by end user. And the shades of blue can be seen in the wells with the four most concentrated human IL-20 standard solutions; the other wells show no obvious color).
9. Add 0.1ml of prepared TMB stop solution into each well. The color changes into yellow immediately.
10. Read the O.D. absorbance at 450nm in a microplate reader within 30 min after adding the stop solution.



Tel: +44-1223-859-353 **Fax:** +44-1223-280-240
Email: info@biorbyt.com **VAT Nr.:** GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 **Fax:** +1-415-651-8558
Email: info@biorbyt.com **EIN:** 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States



For calculation, (the relative O.D.450) = (the O.D.450 of each well) – (the O.D.450 of Zero well). The standard curve can be plotted as the relative O.D.450 of each standard solution (Y) vs. the respective concentration of the standard solution (X). The human IL-20 concentration of the samples can be interpolated from the standard curve. **Note:** if the samples measured were diluted, multiply the dilution factor to the concentrations from interpolation to obtain the concentration before dilution.

Summary

1. Add samples and standards and incubate the plate at 37°C for 90 min. Do not wash.
2. Add biotinylated antibodies and incubate the plate at 37°C for 60 min. Wash plate 3 times with 0.01M TBS.
3. Add ABC working solution and incubate the plate at 37°C for 30 min. Wash plate 5 times with 0.01M TBS.
4. Add TMB color developing agent and incubate the plate at 37°C in dark for 20-25 min.
5. Add TMB stop solution and read.

Background

Interleukin-20 (IL-20) is a protein belonging to the IL-10 family of cytokines. IL-20 is produced by activated keratinocytes and monocytes and transmits an intracellular signal through two distinct cell-surface receptor complexes on keratinocytes and other epithelial cells. By radiation hybrid analysis, the IL20 gene was mapped to chromosome 1q32, where it is tightly linked to the IL10, IL19, and MDA7 genes within a 195 -kb region, the IL10 family cytokine cluster. IL-20 regulates proliferation and differentiation of keratinocytes during inflammation, particularly inflammation associated with the skin. In addition, IL-20 also causes cell expansion of multipotential hematopoietic progenitor cells.



Tel: +44-1223-859-353 Fax: +44-1223-280-240
Email: info@biorbyt.com VAT Nr.: GB 991815777

Biorbyt Ltd
5 Orwell Furlong, Cambridge, CB4 0WY, United Kingdom
Company No. 7479871, registered in England and Wales



Tel: +1-415-906-5211 Fax: +1-415-651-8558
Email: info@biorbyt.com EIN: 33-1226022

Biorbyt LLC
220 Montgomery Street, Suite 810
San Francisco, CA, 94104, United States

